



ExoELISA-ULTRA CD63 Kit

Cat# EXEL-ULTRA-CD63-1

User Manual

See Kit Components for Individual Storage Conditions

Version 3
6/27/2018

A limited-use label license covers this product. By use of this product, you accept the terms and conditions outlined in the License and Warranty Statement contained in this user manual.

Contents

Product Description.....	1
List of Components.....	1
Storage.....	1
Equipment to be supplied by user.....	1
Protocol:	2
Exosome Precipitation.....	2
Sample Preparation	2
Exosome Protein Standard Curve.....	2
ExoELISA Procedure.....	4
Before starting.....	4
ELISA assay.....	4
Example Data and Applications.....	5
Next Steps and Related Products	5
Technical Support.....	6
Licensing and Warranty Statement	6

Product Description

The ExoELISA-ULTRA CD63 assay is a sensitive, direct Enzyme-Linked ImmunoSorbent Assay (ELISA) to quantitate exosome abundance in a given sample that can be performed within 4 hours, start to finish. Exosomes are captured intact on the high protein binding microtiter plate. The wells are incubated with an anti-CD63 primary antibody which recognizes the tetraspanin protein on the exosomal surface. A Horseradish Peroxidase enzyme linked secondary antibody is used for signal amplification. A colorimetric substrate (extra-sensitive TMB) is used for the assay read-out. The accumulation of the colored product is proportional to the amount of specific CD63 antigen present in each well. The results are quantitated by a microtiter plate reader at 450 nm absorbance.

List of Components

COMPONENT	AMOUNT	STORAGE
Anti-CD63 Primary Antibody	60 uL	-20°C
HRP-conjugated Secondary Antibody	10 uL	-20°C
ExoELISA-ULTRA protein standard	4 uL	-20°C
Blocking Buffer	10 mL	4°C
Coating Buffer	20 mL	4°C
Wash Buffer (20X)	10 mL	4°C
ELISA Substrate	6 mL	4°C
Stop Buffer	6 mL	RT
ELISA plate	1	RT

Storage

The kits are shipped at blue ice or dry ice. Individual kit components are stored at different temperatures. Please review the kit component list carefully. Properly stored kits are stable for 6 months from the date received.

Equipment to be supplied by user

1. Microtiter plate sealing film/cover
2. 37°C incubator
3. Microtiter plate shaker
4. Microtiter plate spectrophotometer with 450 nm absorbance capability
5. Multichannel pipets (recommended)

Protocol:

Exosome Precipitation

For simple and quick isolation of exosomes from serum, we recommend using the ExoQuick precipitation solution (Catalog# EXOQ5A-1 or EXOQ20A-1) and the ExoQuick-TC/CG for isolation of exosomes from tissue culture media and urine samples (EXOTC10A-1 or EXOTC50A-1) using the recommend protocols. Resuspend the pellet in sterile DPBS.

Sample Preparation

The recommended input of protein equivalent of exosomes will vary depending on the biofluid and exosome isolation method. For ExoQuick and ExoQuick-TC isolation, we recommend using 1-200ug of protein input/well for the ExoELISA-ULTRA assay.

1. Use an input of 1-200ug protein equivalent of exosomes/well. The assay signal strength is dependent on the expression level of CD63 on the exosome membrane.
2. Make up the volume of exosomes (resuspended in sterile DPBS) to 120uL with the Coating Buffer (sufficient for duplicate wells).

Exosome Protein Standard Curve


A standard curve should be prepared each time the assay is performed. ***DO NOT freeze-thaw diluted standards. Make a fresh dilution of the standards (see Step 2, below) each time the assay is performed.***

1. Thaw ExoELISA-ULTRA protein standard on ice
2. Dilute ExoELISA-ULTRA protein standard 1:1000 in Coating Buffer in a microcentrifuge tube first (for example, add 1uL Standard to 1mL Coating Buffer). Vortex to mix well. Use this dilution as the First Standard for the standard curve.
3. Perform serial dilutions of the First Standard in Coating Buffer in microcentrifuge tubes. Vortex to mix well after each dilution.
4. Suggested dilutions for making the ExoELISA-ULTRA standard curve are shown below. To run the standards in duplicate, double the recipes listed and split into two separate wells.
5. ***Discard the diluted standards after use, do not freeze-thaw or reuse any of the diluted standards.***

Suggested Dilutions – Standard Curve

Tube	Exosome Abundance	Dilution factor	ExoELISA-ULTRA protein standard	Coating buffer
0	0	Blank	-	60 µl
1	4.56×10^{10}	1	1000µl	-
2	2.28×10^{10}	1:2	60 µl	60 µl
3	1.14×10^{10}	1:4	60 µl	60 µl
4	5.7×10^9	1:8	60 µl	60 µl
5	2.9×10^9	1:16	60 µl	60 µl
6	1.4×10^9	1:32	60 µl	60 µl
7	7×10^8	1:64	60 µl	60 µl

ExoELISA-ULTRA Standards calibrated by NanoSight

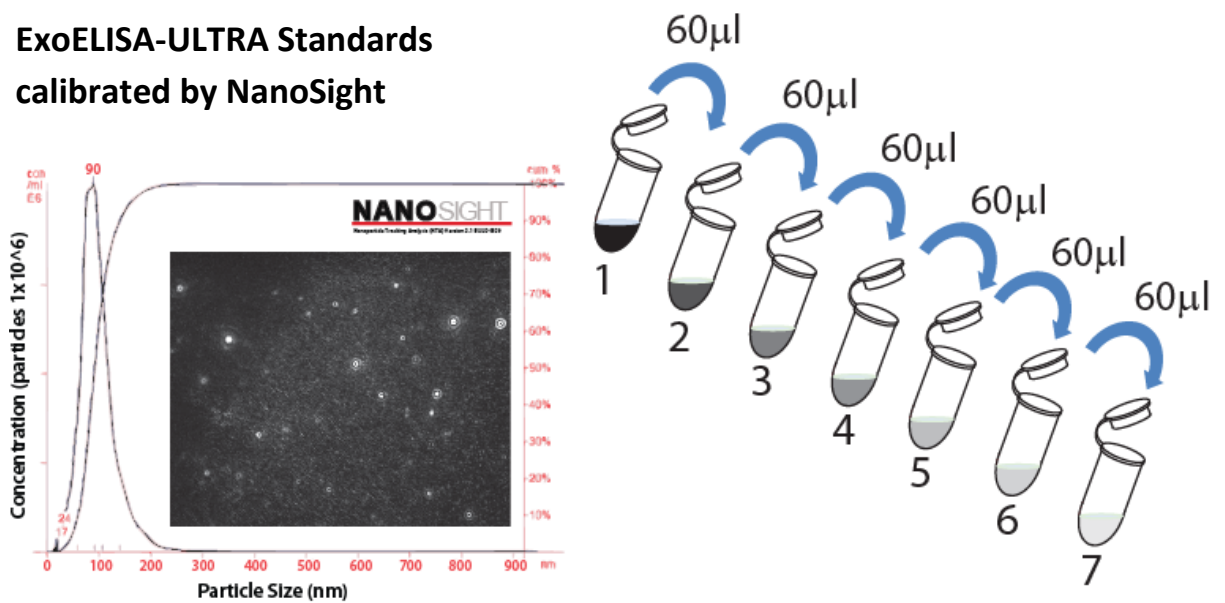

ExoELISA Procedure

Before starting


1. Make sure to warm the **Super-sensitive TMB ELISA** substrate to room temperature before adding to the ELISA plate wells in step #10.
2. Dilute stock **20X Wash buffer** into **1X working Wash buffer** with purified water (each 8-well column requires approximately 10 ml of 1X Wash buffer solution).

ELISA assay

1. Add 50 µl of freshly prepared protein standards (see protocol above) and exosome samples to the appropriate well of the micro-titer plate.
2. Cover plate with sealing film/cover.
3. Incubate the plate at 37°C for 1h.
4. After incubation step, invert the plate to empty all contents.
5. Wash the plate 3 times for 5 minutes each with 100 µl **1X Wash buffer**.
 - A micro-titer plate shaker is recommend for all subsequent washing and incubation steps.
 - Residual liquid should be removed by hard-tapping the plate on fresh paper towels, while taking care not to let the wells dry out completely.
6. Dilute the **CD63 primary antibody** using the ratio 1:100 in Blocking Buffer and add 50 µl of to each well.
7. Incubate the plate at room temperature for 1 hour with shaking.
8. Wash the plate 3 times for 5 minutes each with 100 µl **1X Wash buffer**.
9. Dilute the **secondary antibody** 1:5,000 in Blocking Buffer and add 50 µl to each well.
10. Incubate the plate at room temperature for 1 hour with shaking.
11. Wash the plate 3 times for 5 minutes each with 100 µl **1X Wash buffer**.
12. Add 50 µl of **Super-sensitive TMB ELISA** substrate and incubate at room temperature for 5- 15 mins with shaking*. Add 50 µl of **Stop buffer** and **read immediately** to provide a fixed endpoint for the assay. *The initial color of a positive sample is blue and the color changes to yellow when Stop Buffer is added.*
13. Quantitate results with a spectrophotometric plate reader at 450 nm.

* **Note: Optimal incubation time is dependent on lab conditions and/or instrument used. We strongly suggest running a sample set of standards to optimize the assay prior to running sensitive samples. This will help you determine the optimal conditions for your experiment.**

Example Data and Applications

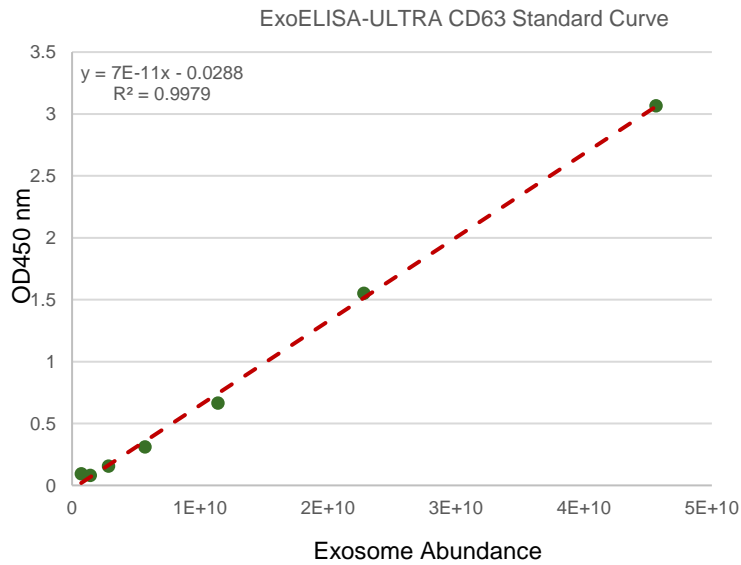

Next Steps and Related Products

Application	Related Products	Website links
Precipitation of Exosomes from other biological fluids		
Exosome Isolation from Tissue Culture Media	ExoQuickTC	https://www.systembio.com/microrna-research/exoquick-exosomes/ordering
Exosome Isolation from Plasma	ExoQuick Plasma prep and Exosome precipitation kit	https://www.systembio.com/microrna-research/exoquick-exosomes/ordering
Protein Characterization of Exosomes		
Western blotting	Exosome antibodies	https://www.systembio.com/microrna-research/exosome-antibody/exoab
Antibody Arrays	ExoCheck Assays	https://www.systembio.com/microrna-research/exosome-antibody-arrays
Quantification of Exosomes		
Quantification of exosomes	EXOCET Assays	https://www.systembio.com/microrna-research/exosome-antibody/exocet-assay
RNA extraction from Exosomes		
RNA extraction and profiling	SeraMir kits	https://www.systembio.com/microrna-research/seramir-exosome-rna-profiling/overview

Technical Support

For more information about SBI products and to download manuals in PDF format, please visit our web site:
<http://www.systembio.com>

For additional information or technical assistance, please call or email us at:

System Biosciences (SBI)
2438 Embarcadero Way
Palo Alto, CA 94303

Phone: (650) 968-2200
(888) 266-5066 (Toll Free)

Fax: (650) 968-2277

E-mail:

General Information: info@systembio.com
Technical Support: tech@systembio.com
Ordering Information: orders@systembio.com

Licensing and Warranty Statement

Limited Use License

Use of the ExoELISA-Ultra Kits (*i.e.*, the “Product”) is subject to the following terms and conditions. If the terms and conditions are not acceptable, return all components of the Product to System Biosciences (SBI) within 7 calendar days. Purchase and use of any part of the Product constitutes acceptance of the above terms.

The purchaser of the Product is granted a limited license to use the Product under the following terms and conditions:

- The Product shall be used by the purchaser for internal research purposes only. The Product is expressly not designed, intended, or warranted for use in humans or for therapeutic or diagnostic use.
- The Product may not be resold, modified for resale, or used to manufacture commercial products without prior written consent of SBI.
- This Product should be used in accordance with the NIH guidelines developed for recombinant DNA and genetic research.

SBI has pending patent applications related to the Product. For information concerning licenses for commercial use, contact SBI.

Purchase of the product does not grant any rights or license for use other than those explicitly listed in this Licensing and Warranty Statement. Use of the Product for any use other than described expressly herein may be covered by patents or subject to rights other than those mentioned. SBI disclaims any and all responsibility for injury or damage which may be caused by the failure of the buyer or any other person to use the Product in accordance with the terms and conditions outlined herein.

Limited Warranty

SBI warrants that the Product meets the specifications described in this manual. If it is proven to the satisfaction of SBI that the Product fails to meet these specifications, SBI will replace the Product or provide the purchaser with a refund. This limited warranty shall not extend to anyone other than the original purchaser of the Product. Notice of nonconforming products must be made to SBI within 30 days of receipt of the Product.

SBI's liability is expressly limited to replacement of Product or a refund limited to the actual purchase price. SBI's liability does not extend to any damages arising from use or improper use of the Product, or losses associated with the use of additional materials or reagents. This limited warranty is the sole and exclusive warranty. SBI does not provide any other warranties of any kind, expressed or implied, including the merchantability or fitness of the Product for a particular purpose.

SBI is committed to providing our customers with high-quality products. If you should have any questions or concerns about any SBI products, please contact us at (888) 266-5066.

© 2018 System Biosciences (SBI), All Rights Reserved



System Biosciences (SBI)
2438 Embarcadero Way
Palo Alto, CA 94303

Phone: (650) 968-2200
Toll Free (888) 266-5066
Fax: (650) 968-2277

E-mail:

General Information: info@systembio.com
Technical Support: tech@systembio.com
Ordering Information: orders@systembio.com